


Overview

Sample 2013-01: CT positive/NG negative

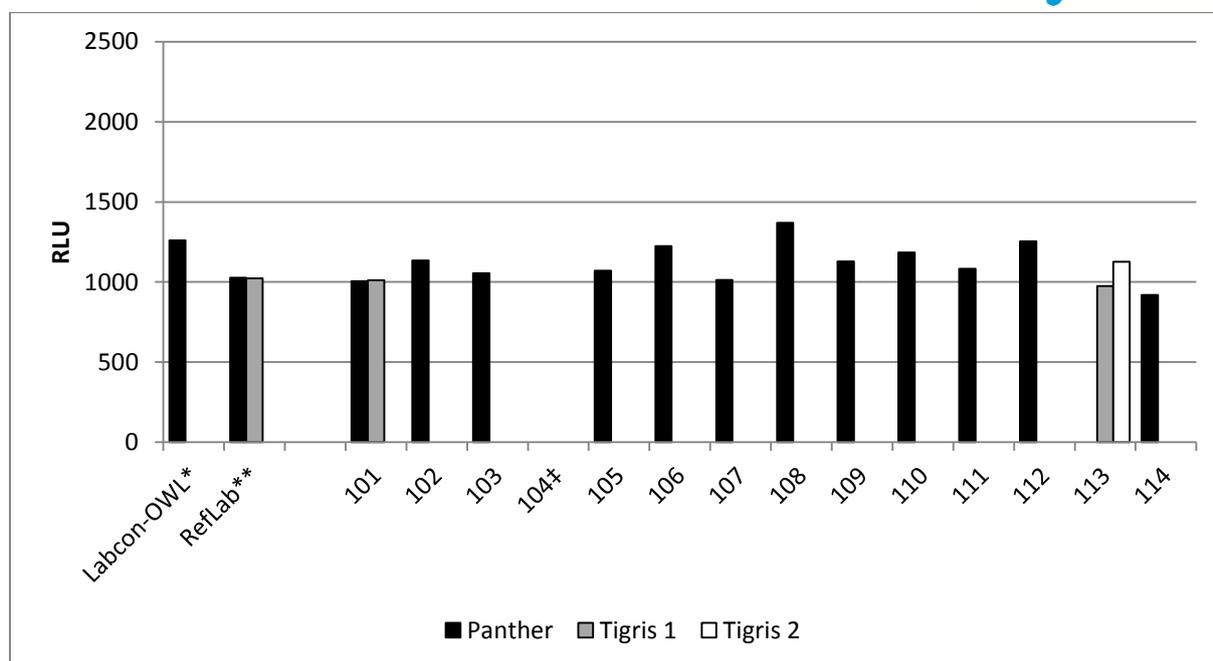

	RLU Panther	RLU Tigris 1	RLU Tigris 2
<b>Labcon-OWL</b>	1260		
<b>RefLab</b>	1027	1022	
<b>101</b>	1005	1010	-
<b>102</b>	1134	-	-
<b>103</b>	1054	-	-
<b>104</b>	-	-	-
<b>105</b>	1071	-	-
<b>106</b>	1225	-	-
<b>107</b>	1013	-	-
<b>108</b>	1370	-	-
<b>109</b>	1129	-	-
<b>110</b>	1184	-	-
<b>111</b>	1082	-	-
<b>112</b>	1254	-	-
<b>113</b>	-	975	1126
<b>114</b>	920	-	-


\*Average RLU value determined over the entire period of the external quality assessment by Labcon-OWL

\*\*Reference laboratory HOLOGIC GEN-PROBE (USA)

‡No information about RLU values



Sample 2013-02: CT/NG negative

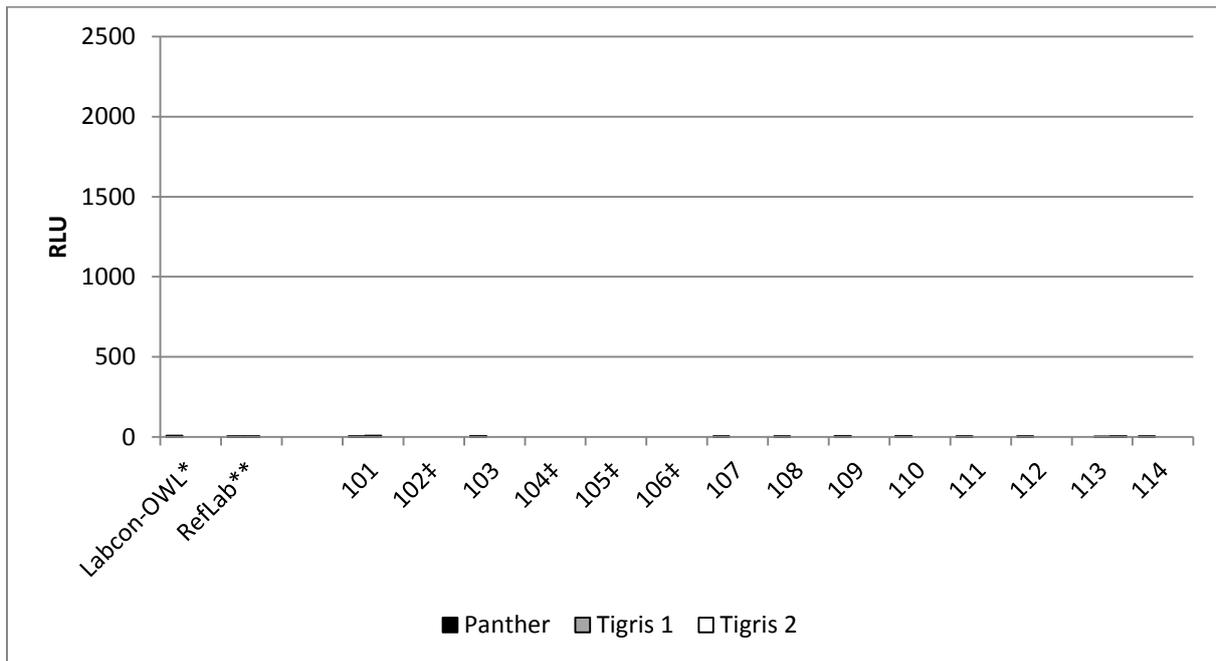


	RLU Panther	RLU Tigris 1	RLU Tigris 2
<b>Labcon-OWL</b>	8		
<b>RefLab</b>	4	5	
<b>101</b>	5	8	-
<b>102</b>	-	-	-
<b>103</b>	7	-	-
<b>104</b>	-	-	-
<b>105</b>	-	-	-
<b>106</b>	-	-	-
<b>107</b>	5	-	-
<b>108</b>	5	-	-
<b>109</b>	6	-	-
<b>110</b>	7	-	-
<b>111</b>	5	-	-
<b>112</b>	5	-	-
<b>113</b>	-	3	5
<b>114</b>	4	-	-

\*Average RLU value determined over the entire period of the external quality assessment by Labcon-OWL

\*\*Reference laboratory HOLOGIC GEN-PROBE (USA)

‡No information about RLU values

## Sample 2013-03: CT/NG positive

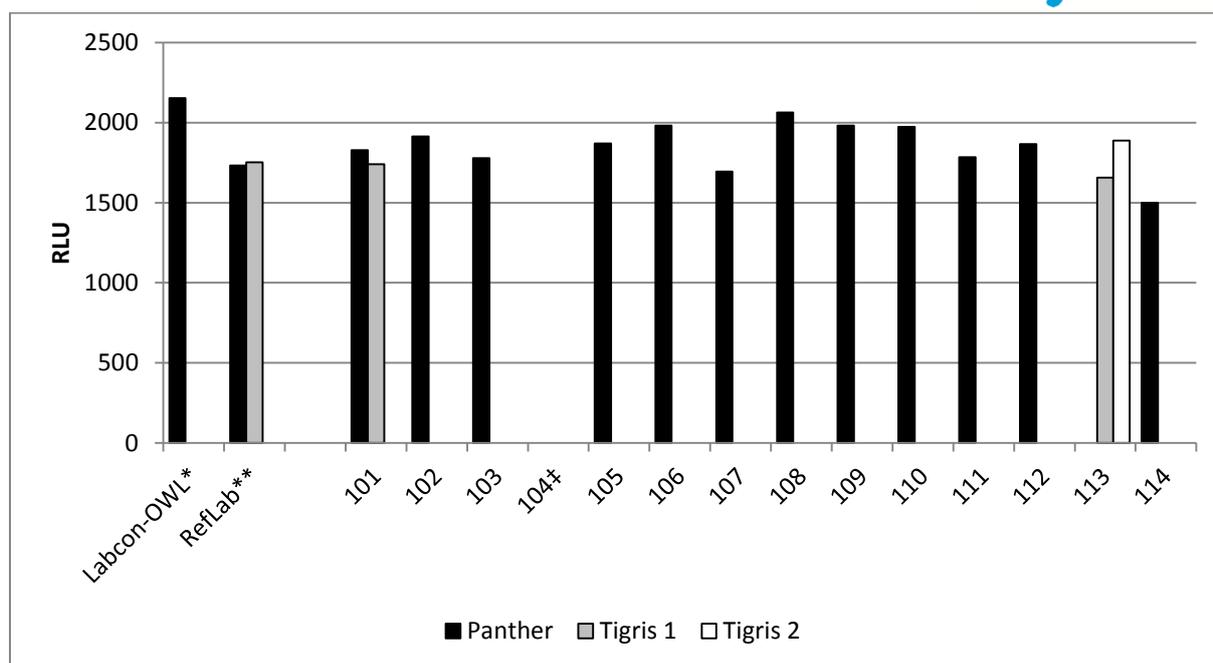


	Panther	Tigris 1	Tigris 2
<b>Labcon-OWL</b>	2152	-	-
<b>RefLab</b>	1733	1753	-
<b>101</b>	1827	1741	-
<b>102</b>	1913	-	-
<b>103</b>	1778	-	-
<b>104</b>	-	-	-
<b>105</b>	1869	-	-
<b>106</b>	1982	-	-
<b>107</b>	1694	-	-
<b>108</b>	2062	-	-
<b>109</b>	1981	-	-
<b>110</b>	1973	-	-
<b>111</b>	1784	-	-
<b>112</b>	1866	-	-
<b>113</b>	-	1657	1888
<b>114</b>	1500	-	-

\*Average RLU value determined over the entire period of the external quality assessment by Labcon-OWL

\*\*Reference laboratory HOLOGIC GEN-PROBE (USA)

‡No information about RLU values

## Sample 2013-04: CT negative/NG positive

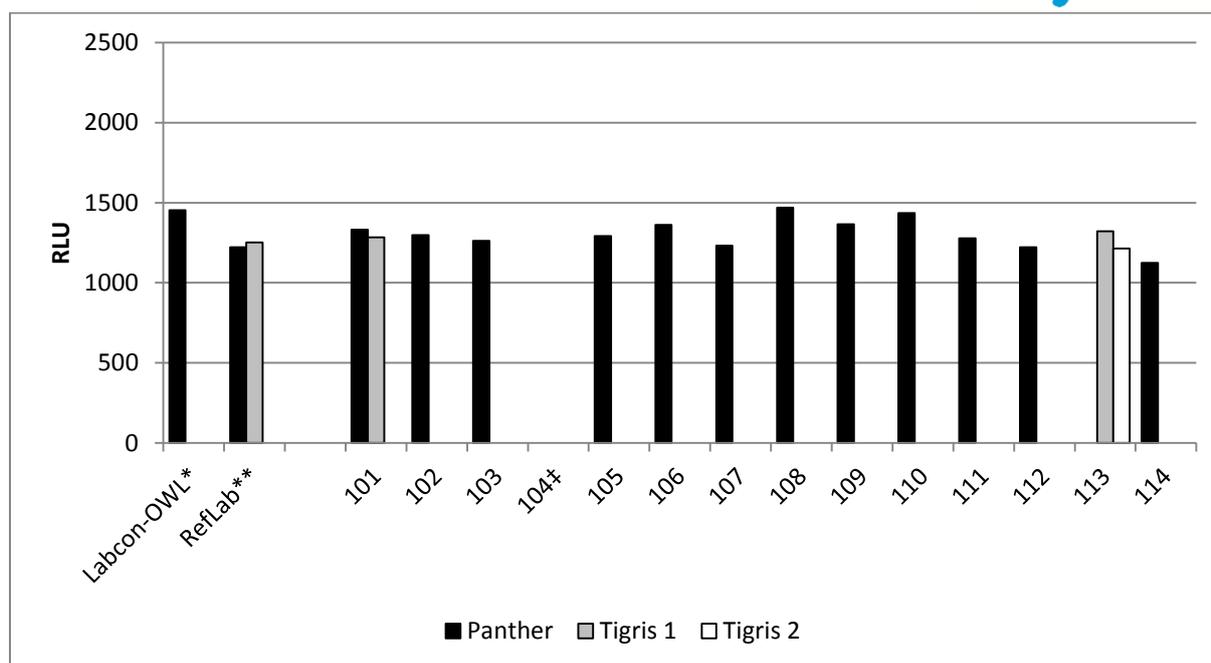

	Panther	Tigris 1	Tigris 2
<b>Labcon-OWL</b>	1453	-	-
<b>RefLab</b>	1223	1251	-
<b>101</b>	1331	1284	-
<b>102</b>	1298	-	-
<b>103</b>	1262	-	-
<b>104</b>	-	-	-
<b>105</b>	1292	-	-
<b>106</b>	1361	-	-
<b>107</b>	1233	-	-
<b>108</b>	1470	-	-
<b>109</b>	1366	-	-
<b>110</b>	1435	-	-
<b>111</b>	1278	-	-
<b>112</b>	1222	-	-
<b>113</b>	-	1322	1215
<b>114</b>	1125	-	-

\*Average RLU value determined over the entire period of the external quality assessment by Labcon-OWL

\*\*Reference laboratory HOLOGIC GEN-PROBE (USA)

‡No information about RLU values