


Overview EQA II/2016



Sample 2016-05: CT negative / NG negative

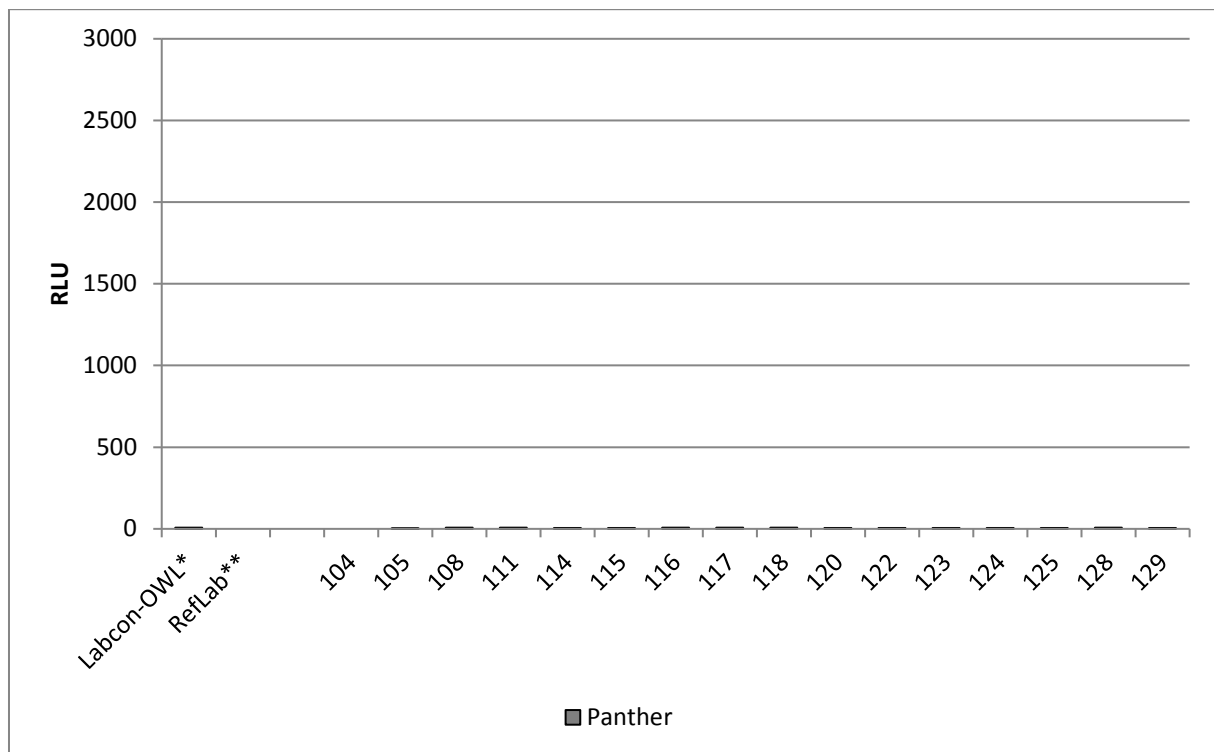


	RLU Panther
Labcon-OWL*	7
RefLab**	0
104	0
105	4
108	7
111	7
114	5
115	6
116	7
117	7
118	7
120	6
122	6
123	5
124	5
125	5
128	8
129	5

*RLU value constantly monitored over the entire testing phase of the external quality assessment by Labcon-OWL

**External Reference Laboratory in Germany


Sample 2016-06: CT positive / NG positive

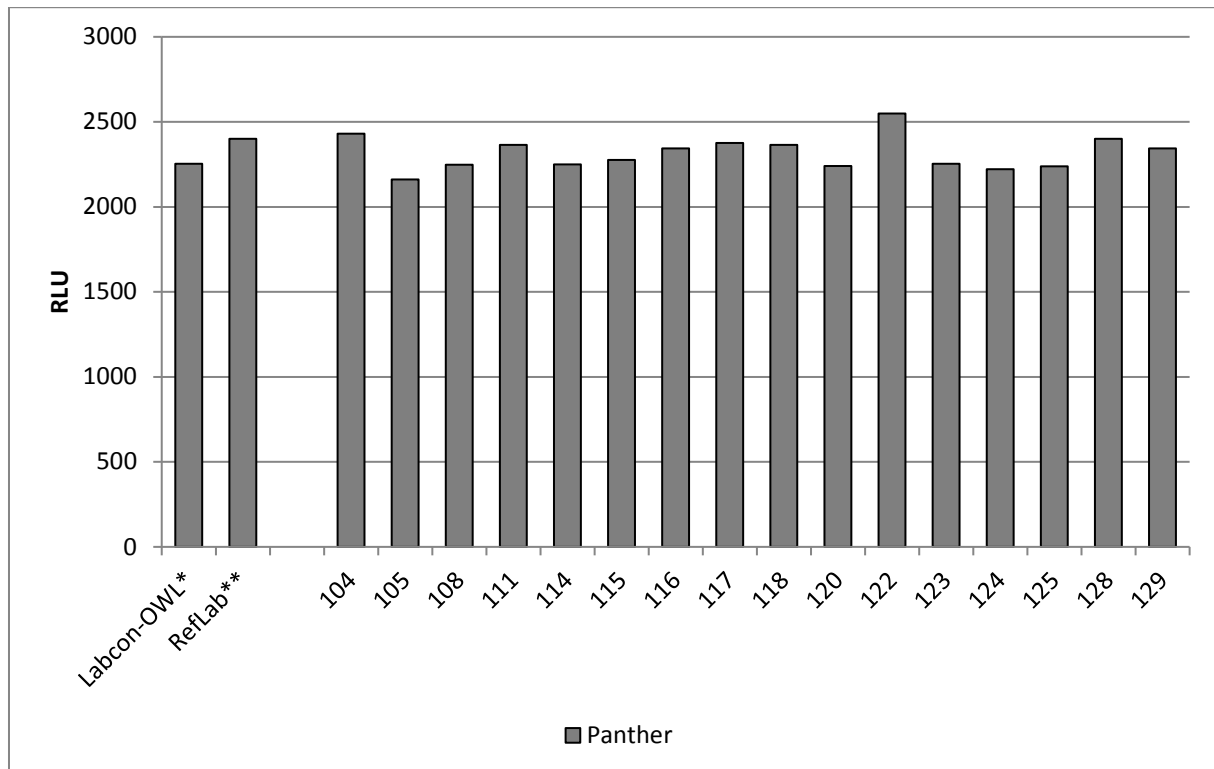

	RLU Panther
Labcon-OWL*	2253
RefLab**	2400
104	2431
105	2161
108	2247
111	2365
114	2250
115	2276
116	2344
117	2376
118	2365
120	2240
122	2549
123	2253
124	2222
125	2238
128	2400
129	2344

*RLU value constantly monitored over the entire testing phase of the external quality assessment by Labcon-OWL

**External Reference Laboratory in Germany

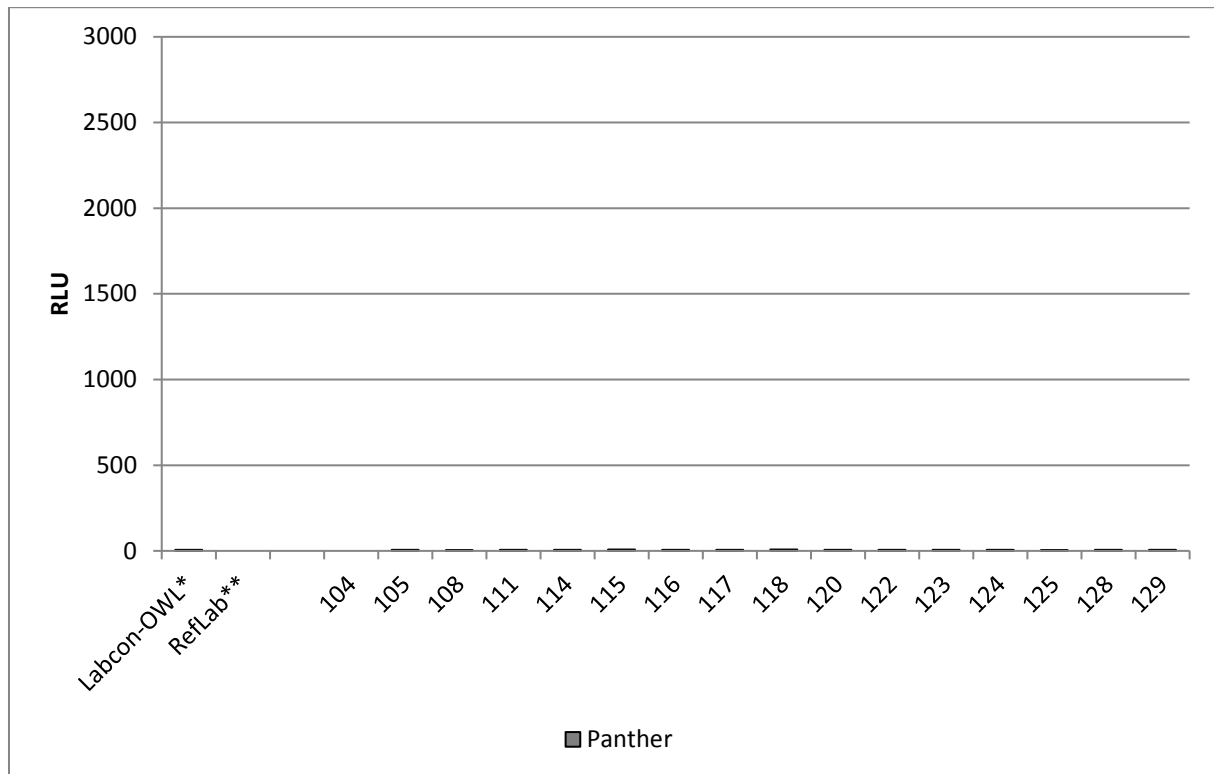
Sample 2016-07: CT negative / NG negative

	RLU Panther
Labcon-OWL*	7
RefLab**	0
104	0
105	7
108	5
111	6
114	6
115	8
116	6
117	7
118	8
120	7
122	7
123	6
124	6
125	5
128	7
129	6

*RLU value constantly monitored over the entire testing phase of the external quality assessment by Labcon-OWL

**External Reference Laboratory in Germany

Sample 2016-08: CT negative / NG positive

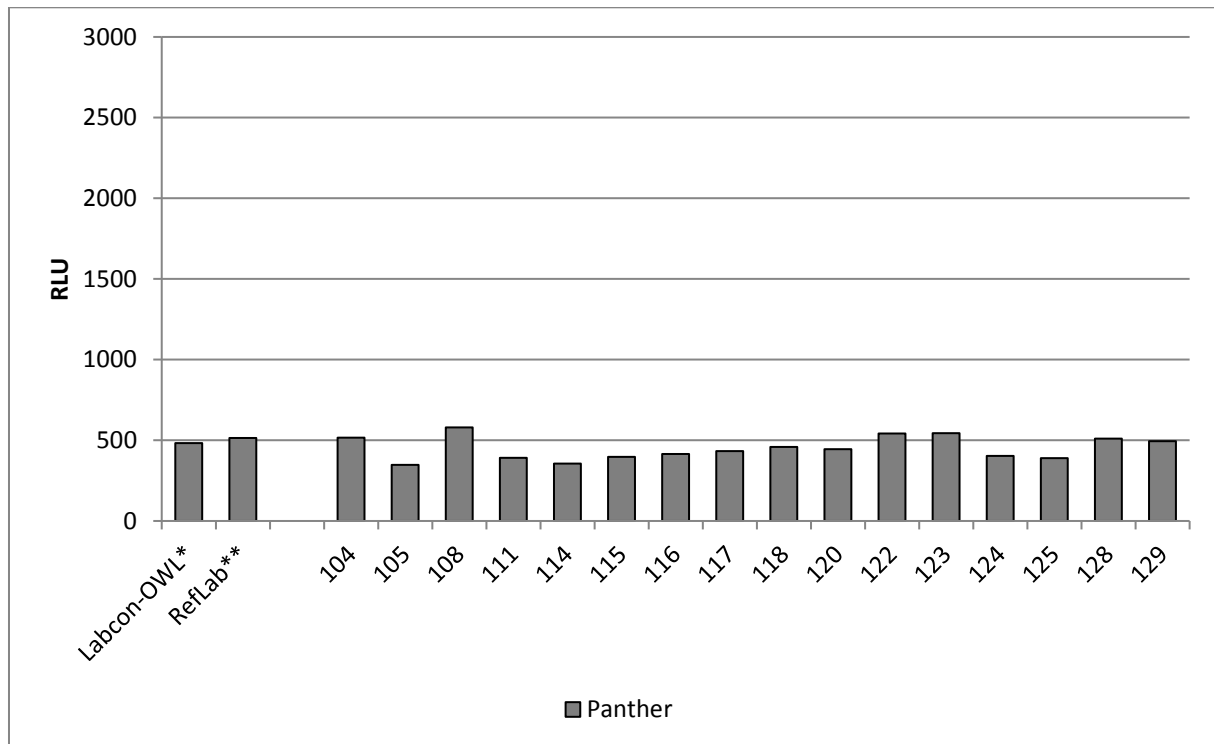


	RLU Panther
Labcon-OWL*	482
RefLab**	515
104	516
105	347
108	579
111	391
114	355
115	397
116	415
117	434
118	458
120	444
122	542
123	544
124	404
125	390
128	511
129	494

*RLU value constantly monitored over the entire testing phase of the external quality assessment by Labcon-OWL

**External Reference Laboratory in Germany

Appendix: Stability of the samples over the period of the external quality assessment

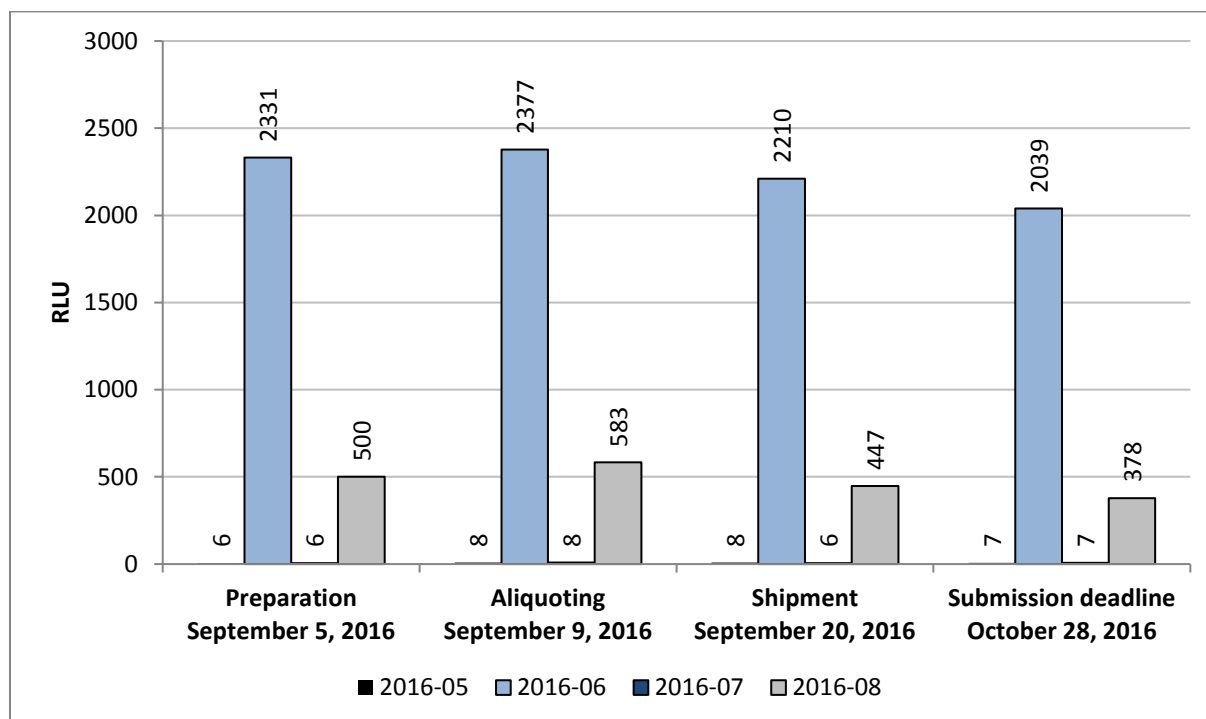

RLU values determined over the period of the external quality assessment by Labcon-OWL

The target value of all samples was confirmed and monitored in a reference laboratory in Germany before distribution. During the testing period the samples were retested three times by Labcon-OWL. The data are illustrated above. This graph shows the course of signal change for all four panel members over a period of seven weeks (storage at room temperature).