


Overview EQA II/2021


Sample 2021-05: CT positive / NG negative

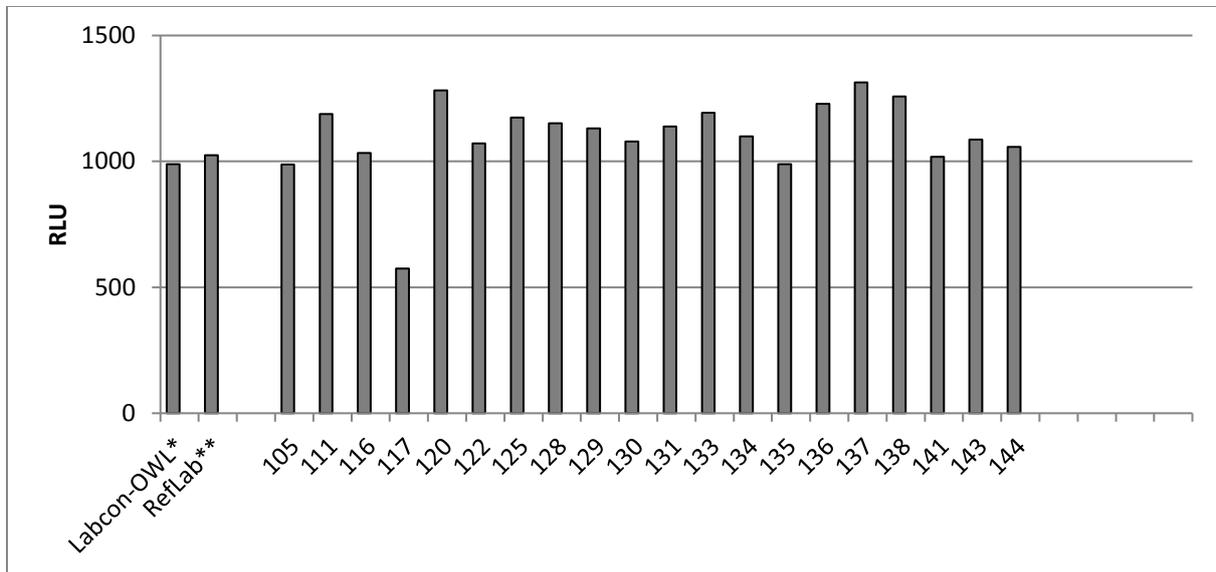

	RLU Panther
<b>LABCON-OWL *</b>	<b>989</b>
<b>RefLab**</b>	<b>1024</b>
<b>105</b>	<b>988</b>
<b>111</b>	<b>1188</b>
<b>116</b>	<b>1033</b>
<b>117</b>	<b>574</b>
<b>120</b>	<b>1282</b>
<b>122</b>	<b>1072</b>
<b>125</b>	<b>1174</b>
<b>128</b>	<b>1152</b>
<b>129</b>	<b>1131</b>
<b>130</b>	<b>1079</b>
<b>131</b>	<b>1139</b>
<b>133</b>	<b>1193</b>
<b>134</b>	<b>1100</b>
<b>135</b>	<b>989</b>
<b>136</b>	<b>1229</b>
<b>137</b>	<b>1314</b>
<b>138</b>	<b>1258</b>
<b>141</b>	<b>1018</b>
<b>143</b>	<b>1087</b>
<b>144</b>	<b>1058</b>

\*RLU value constantly monitored over the entire testing phase of the external quality assessment by LABCON-OWL GmbH  
 \*\*External Reference Laboratory in Germany

Sample 2021-06: CT negative / NG positive

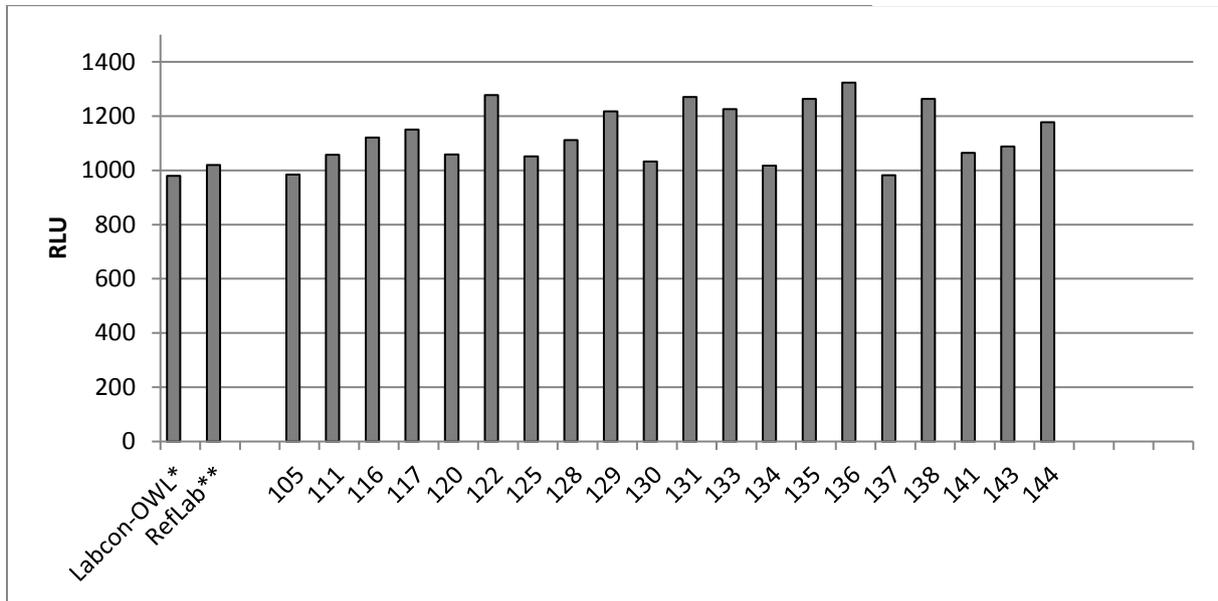


	RLU Panther
<b>LABCON-OWL*</b>	<b>980</b>
<b>RefLab**</b>	<b>1020</b>
<b>105</b>	<b>984</b>
<b>111</b>	<b>1057</b>
<b>116</b>	<b>1121</b>
<b>117</b>	<b>1150</b>
<b>120</b>	<b>1059</b>
<b>122</b>	<b>1277</b>
<b>125</b>	<b>1051</b>
<b>128</b>	<b>1111</b>
<b>129</b>	<b>1218</b>
<b>130</b>	<b>1033</b>
<b>131</b>	<b>1271</b>
<b>133</b>	<b>1226</b>
<b>134</b>	<b>1017</b>
<b>135</b>	<b>1263</b>
<b>136</b>	<b>1324</b>
<b>137</b>	<b>982</b>
<b>138</b>	<b>1263</b>
<b>141</b>	<b>1064</b>
<b>143</b>	<b>1088</b>
<b>144</b>	<b>1178</b>

\*RLU value constantly monitored over the entire testing phase of the external quality assessment by LABCON-OWL

\*\*External Reference Laboratory in Germany

Sample 2021-07: CT negative / NG negative

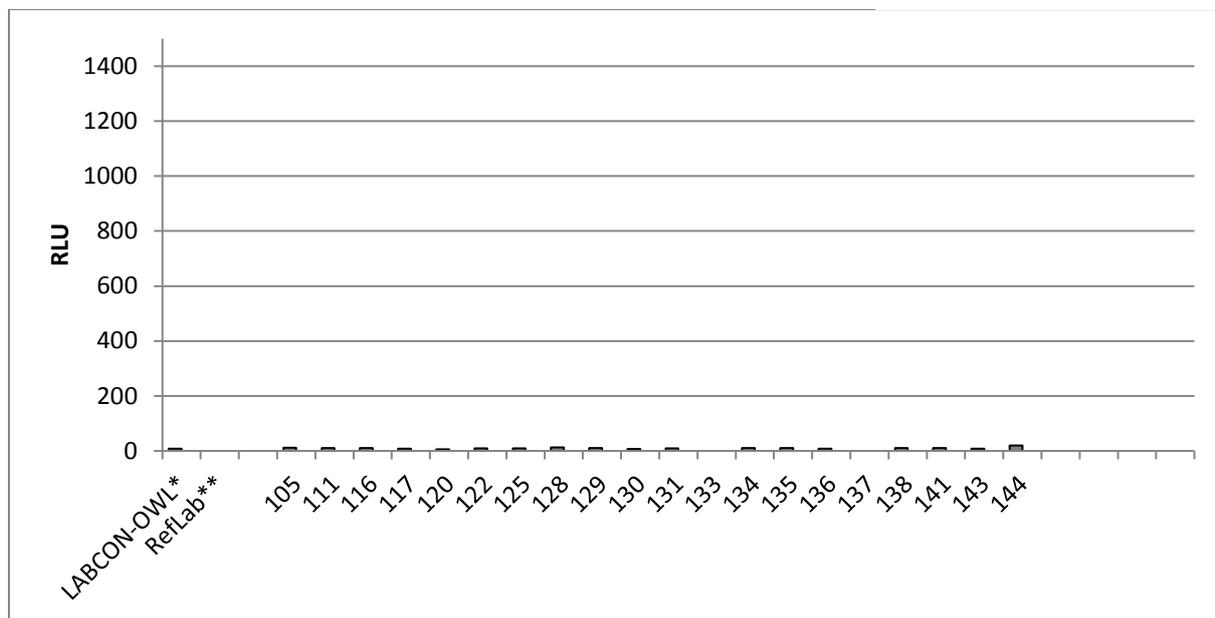


<b>RLU Panther</b>	
<b>LABCON-OWL*</b>	<b>8</b>
<b>RefLab**</b>	<b>0</b>
<b>105</b>	<b>12</b>
<b>111</b>	<b>11</b>
<b>116</b>	<b>10</b>
<b>117</b>	<b>8</b>
<b>120</b>	<b>6</b>
<b>122</b>	<b>9</b>
<b>125</b>	<b>9</b>
<b>128</b>	<b>13</b>
<b>129</b>	<b>10</b>
<b>130</b>	<b>7</b>
<b>131</b>	<b>9</b>
<b>133</b>	<b>0</b>
<b>134</b>	<b>10</b>
<b>135</b>	<b>10</b>
<b>136</b>	<b>8</b>
<b>137</b>	<b>0</b>
<b>138</b>	<b>11</b>
<b>141</b>	<b>10</b>
<b>143</b>	<b>8</b>
<b>144</b>	<b>20</b>

\*RLU value constantly monitored over the entire testing phase of the external quality assessment by LABCON-OWL

\*\*External Reference Laboratory in Germany

Sample 2021-08: CT positive / NG negative

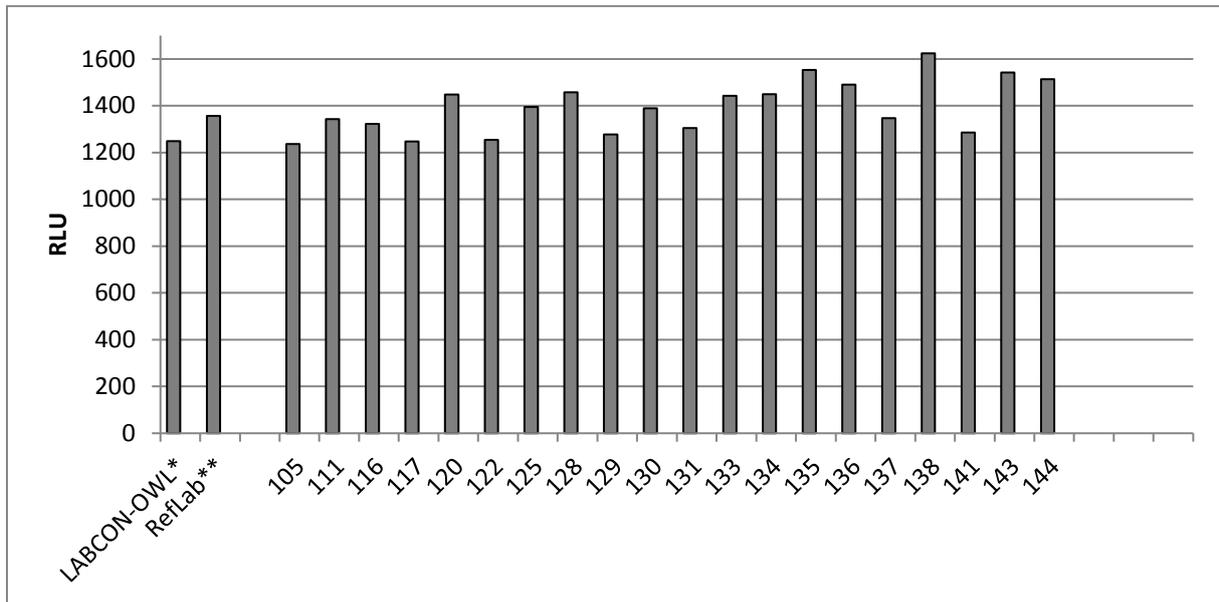


	RLU Panther
LABCON-OWL*	1249
RefLab**	1357
105	1237
111	1343
116	1322
117	1248
120	1448
122	1254
125	1395
128	1457
129	1277
130	1390
131	1305
133	1442
134	1450
135	1553
136	1491
137	1347
138	1624
141	1286
143	1542
144	1514

\*RLU value constantly monitored over the entire testing phase of the external quality assessment by LABCON-OWL

\*\*External Reference Laboratory in Germany



## Appendix: Stability of the samples over the period of the external quality assessment

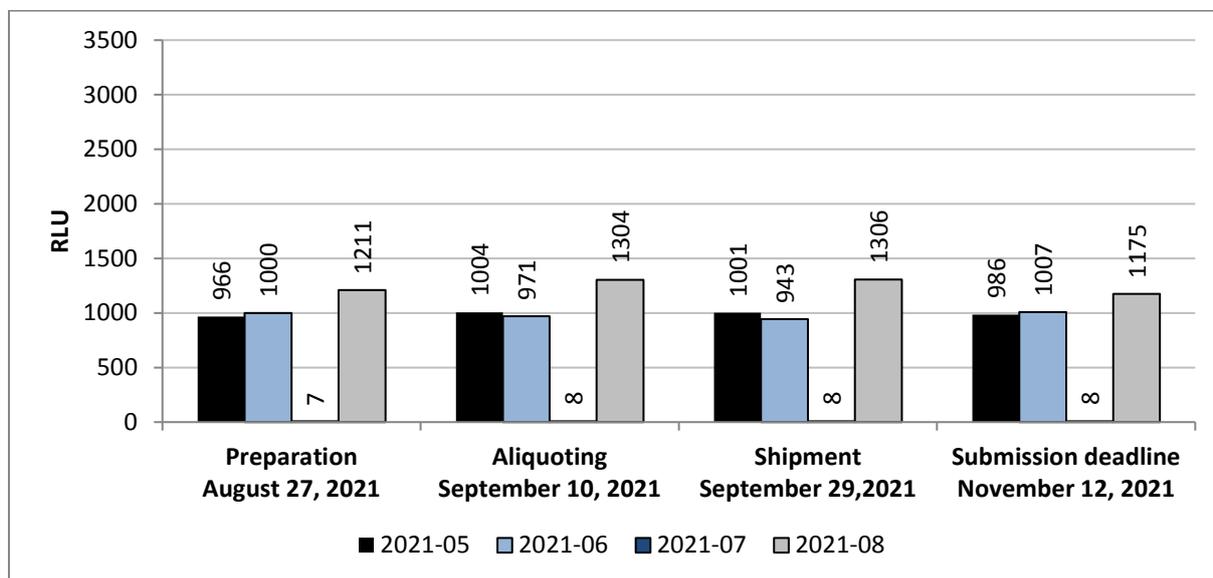

RLU values determined over the period of the external quality assessment by LABCON-OWL

The target value of all samples was confirmed and monitored in a reference laboratory in Germany before distribution. During the testing period the samples were retested three times by LABCON-OWL. The data are illustrated above. This graph shows the course of signal change for all four panel members over a period of eleven weeks (storage at room temperature).